



CONEX-CC

**Single-Axis DC Motion
with Controller/Driver**



 **Newport®**

**Controller GUI
Manual**

V2.0.x

©2018 by Newport Corporation, Irvine, CA. All rights reserved.

Original instructions.

No part of this document may be reproduced or copied without the prior written approval of Newport Corporation. This document is provided for information only, and product specifications are subject to change without notice. Any change will be reflected in future publishings.

Table of Contents

1.0 Introduction	1
1.1 Purpose	1
1.2 Overview	1
1.3 Controller State Diagram.....	2

2.0 Installation.....	3
2.1 Install CONEX-CC Graphical User Interface.....	3
2.2 Launch GUI.....	3

3.0 Getting Started.....	4
3.1 Discover Instruments	4

4.0 User Interface.....	5
4.1 Configuration.....	5
4.2 Main.....	8
4.3 Tracking.....	10
4.4 Diagnostics	12
4.5 About	13

Service Form	15
---------------------------	-----------



Single-Axis DC Motor Controller/Driver CONEX-CC

1.0 Introduction

1.1 Purpose

The purpose of this document is to provide instructions on how to use the CONEX-CC Controller graphical user interface (GUI).

1.2 Overview


The CONEX-CC Controller GUI is a graphical user interface, that allows the user to interact with the CONEX-CC controller that is connected to stages with DC motors and encoder feedback. The user can initiate moves, change the state of the controller, adjust parameters, etc.

1.3 Controller State Diagram

The CONEX-CC controller is defined by the following state diagram.

NOTE

The position tracking is available only from the controller version 2.0.0

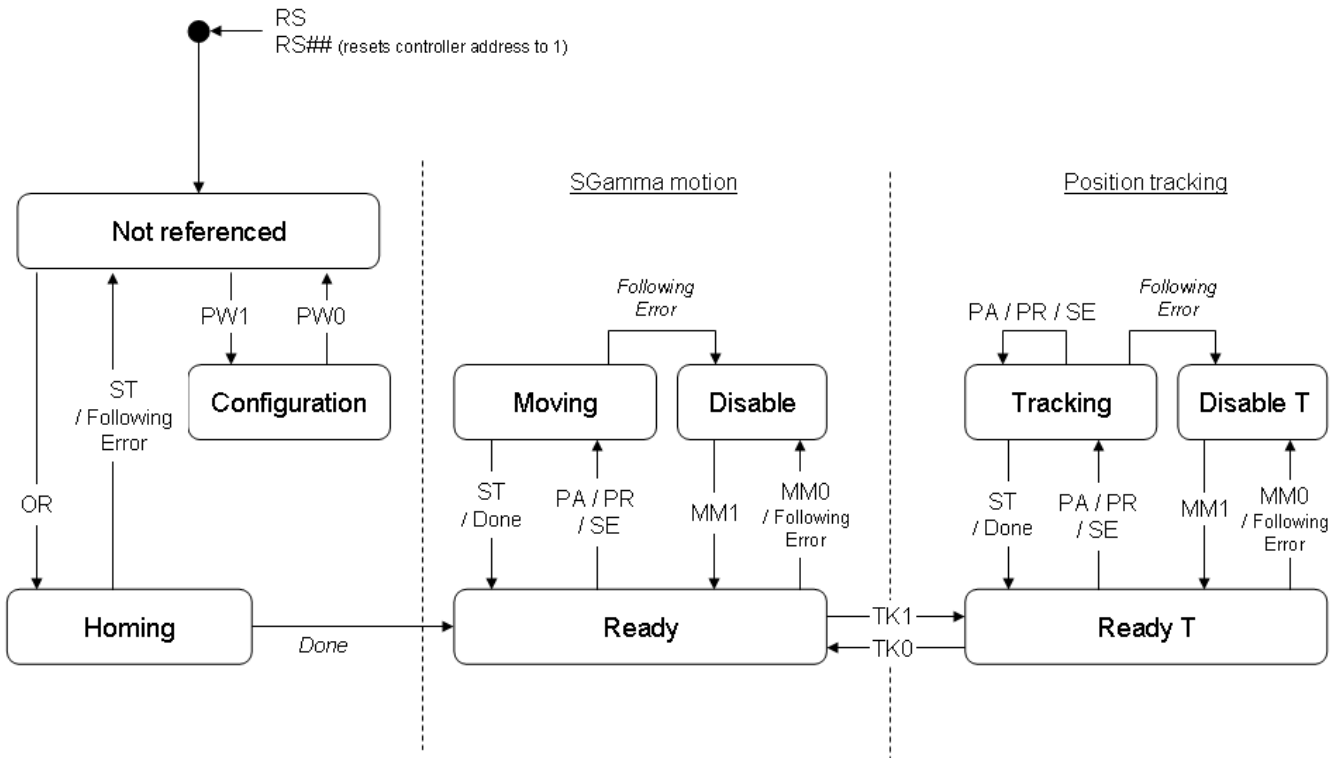

Controller’s LED display:



- NOT REFERENCED: If everything is OK then **SOLID ORANGE**.
- NOT REFERENCED: If hardware faults or wrong parameters then **SOLID RED**.
- NOT REFERENCED: If end of runs then **SLOW BLINK ORANGE**.
- CONFIGURATION: **SLOW BLINK RED**.
- READY / READY T: **SOLID GREEN**.
- DISABLE / DISABLE T: **SLOW BLINK GREEN**.
- HOMING: **FAST BLINK GREEN**.
- MOVING: **FAST BLINK GREEN**.
- TRACKING: **FAST BLINK GREEN**.

2.0 Installation

2.1 Install CONEX-CC Graphical User Interface

Following are steps to install CONEX-CC GUI.

- For 32 bit, Select and launch “CONEX-CC Utility Installer Win32.exe”. For 64 bit, Select and launch “CONEX-CC Utility Installer Win64.exe”.
- A window opens up showing Install welcome page.
- Click on “Next”.
- A window opens up allowing destination folder selection. By default it is showing C:\.
- Click on “Next”.
- Ready to install window opens up. Click “Install”.
- Then installation starts, wait for completion. Click on “Finish” to finalize the installation.

32 bit installer will be installed “Newport.CONEXCC.CommandInterface.dll” in GAC_32 folder and 64 bit installer will be installed the dll in GAC_64 folder.

NOTE

LabVIEW user can add reference of command interface dll from GAC during VI creation.


2.2 Launch GUI

From Windows “START” menu, select “All Programs\Newport\Motion Control\CONEX-CC\CONEXCC Utility”.


3.0 Getting Started

3.1 Discover Instruments

Start the Controller GUI from `Newport\MotionControl\CONEX-CC`.

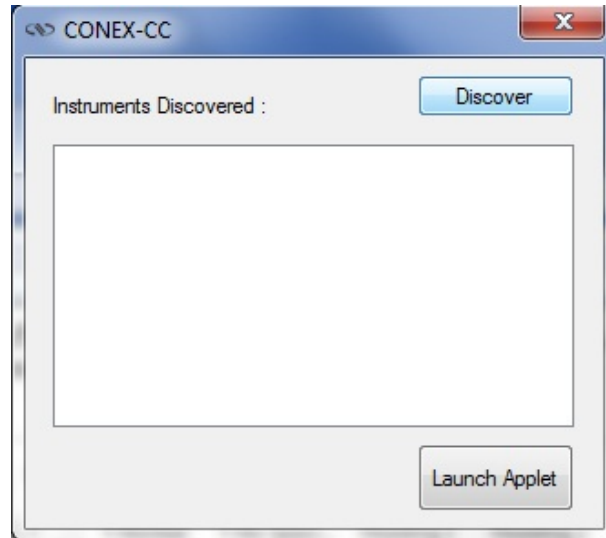

Next, click on “**Discover**” button and the number of instruments discovered will appear. This window allows the user to select a com port where the desired instrument is connected.

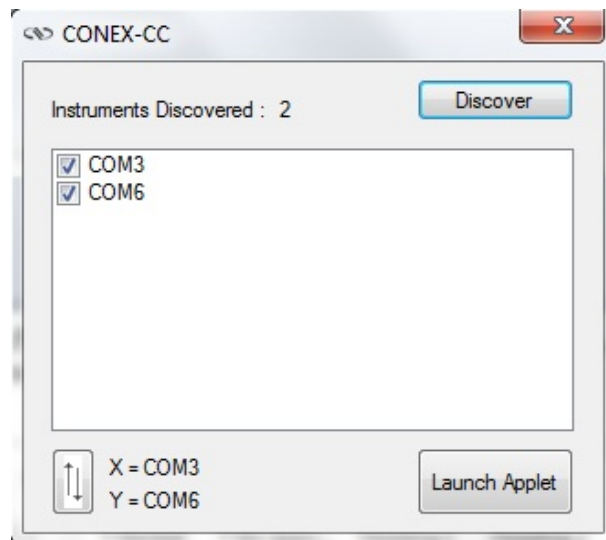

NOTE


When more than one CONEX-CC instrument is connected, this window allows the user to switch the instruments between X and Y axes. To discern a com port for a specific instrument, note their COM number in the Device Manager when the connection is added.

Next, click “**Launch Applet**” button.

4.0 User Interface

4.1 Configuration

The Configuration tab allows the user to view and / or change information related to the logging configuration and the instrument settings. Read only values are displayed for the log file name and the log file path. The logging level may be changed to any of the settings in the drop-down list on the right hand side. Trace is the most detailed of the settings and when this setting is selected the Controller GUI logs everything. Critical Error is the least detailed of the settings and when this setting is selected the Controller GUI will only log errors that are defined to be critical.

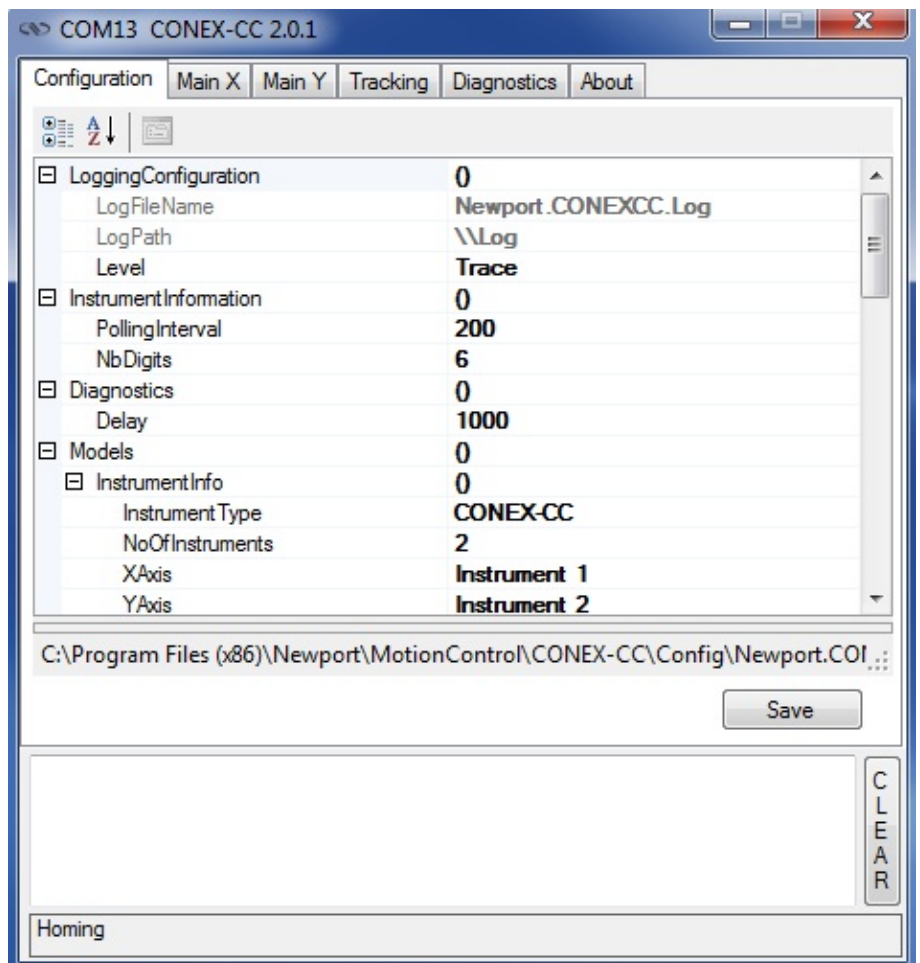

The polling interval defines the number of milliseconds between each time the Controller GUI polls the CONEX-CC for the latest information. The user may change the polling interval by entering a value. Diagnostics Delay defines the time delay in milliseconds between each command sent from a text file.

InstrumentType and NoOfInstruments display the name and number of connected instruments.

The **Save** button allows to save the current settings to the configuration file.

Configurable settings

The following table describes all the settings that can be changed by the user.

Parameter	Description	Values	Default
LoggingConfiguration			
Level	Logging level. Trace is the most detailed of the settings and when this setting is selected the Controller GUI logs everything. Critical Error is the least detailed of the settings and when this setting is selected the Controller GUI will only log errors that are defined to be critical.	Trace Detail Equipment Message Info Warning Error Critical Error	Trace
InstrumentInformation			
PollingInterval	The polling interval defines the number of milliseconds (delay) between each time the Controller GUI polls the instrument for the latest information.	An Integer	200
NbDigits	Number of fractional digits after the decimal point.	An Integer	6
Diagnostic			
Delay	The delay defines the number of milliseconds between each sent command from a text file.	An Integer	5
MemorizePositionsRollingBuffer			
Buffer Depth	BufferDepth defines the maximum number of analog I/O values displayed in the chart.		
Positions	Positions is a list of memorized positions. The format is "Name of positions #1; X position #1; Y position #2..."		
Models\InstrumentInfo			
XAxis	XAxis defines the instrument for X axis. None = no instrument for X axis	Instrument 1 Instrument 2 None	Instrument 1
YAxis	YAxis defines the instrument for Y axis. None = no instrument for Y axis	Instrument 1 Instrument 2 None	Instrument 2
CommunicationChannel	The communication channel	USB	USB
InstrumentType	Specifies type of instrument connected to computer	Name of instrument	
NoOfInstruments	Specifies number of instruments connected to computer	An Integer	0 if nothing is connected
TrackingConfiguration			
XDirection	The axis direction for X axis.	Normal Inverse	Normal
YDirection	The axis direction for Y axis.	Normal Inverse	Normal
StartedSensibility	The started sensibility defines the zoom level of the tracking panel after Controller GUI launching.	An Integer (1<20)	4
MinimumAmplitudeX	The minimum amplitude for X axis.	A Double	0.001
MaximumAmplitudeX	The maximum amplitude for X axis.	A Double	20
MinimumAmplitudeY	The minimum amplitude for Y axis.	A Double	0.001
MaximumAmplitudeY	The maximum amplitude for Y axis.	A Double	20
IncrementalStep	The maximum incremental step when the tracking is in incremental displacement mode.	A Double	0.05

This table describes mouse parameters for the MouseConfiguration section.


MouseConfiguration			
EnterPositionTracking	Activate the tracking mode.	MouseButton/MouseEvent*	Middle/Click
ExitPositionTracking	Desactivate the tracking mode.	MouseButton/MouseEvent*	Middle/Click
SelectXaxis	Select/Unselect X axis.	MouseButton/MouseEvent*	Left/Click
SelectYaxis	Select/Unselect Y axis.	MouseButton/MouseEvent*	Right/Click
IncreaseSensibility	Increase the zoom level of the tracking panel.	MouseButton/MouseEvent*	Middle/Wheel up
DecreaseSensibility	Decrease the zoom level of the tracking panel.	MouseButton/MouseEvent*	Middle/Wheel down
MemorizeCurrentPosition	Save the current positions.	MouseButton/MouseEvent*	Left/Double-Click

4.2 Main

The Main tab displays the main controls in the Controller GUI like a virtual front panel. It is updated each time the polling interval timer expires.

One Main tab by axis:

1. Main X
2. Main Y

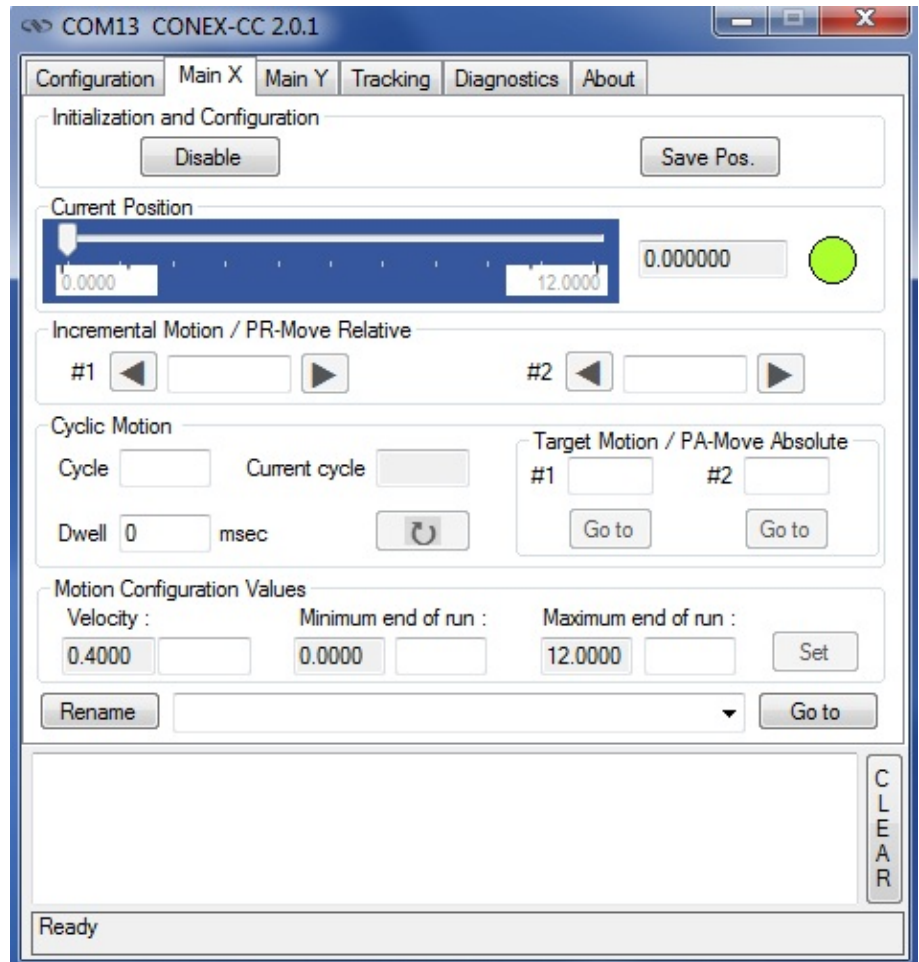

“Initialization and Configuration”

In the “Initialization and Configuration” area, the first button changes the controller status to “Enabled” or “Disabled”. To see the different controller states, refer to the controller state diagram in section 1.3. The second button “Save Pos.” memorizes the current positions (X and Y) in the combo box. As soon as a new position is memorized, this is displayed in the trace.

“Current Position”


In the “Current Position” area, the current position X (or Y) is displayed in a text box and visualized in a slider. The slider limits are defined with the ends of run. An LED icon shows the current controller state. When the mouse hovers over the LED icon, the controller state is displayed in an information balloon.

“Incremental Motion / PR-Move Relative”

In the “Incremental Motion / PR-Move Relative” area, two increment values can be defined. For each defined increment, a relative move is performed in either the negative direction or positive direction.

“Cyclic Motion” and “Target position / PA-Move Absolute”

In the “Cyclic Motion” area, a motion cycle is configured with a number of cycles (Cycle) and a dwell time in milliseconds. The motion cycle gets the defined target positions from the “Target position / PA-Move Absolute” area to perform the cycle.

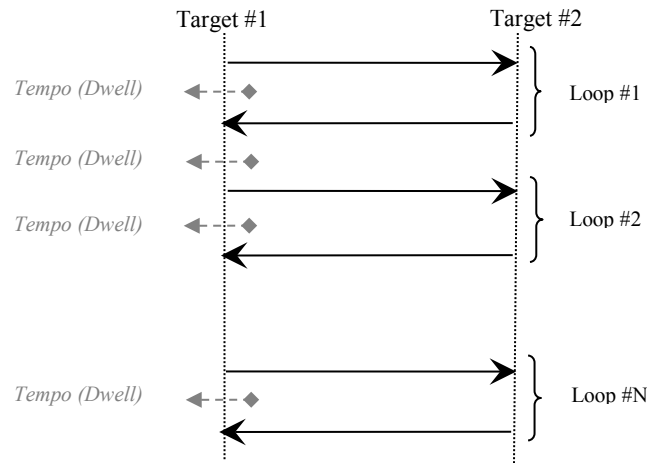

In the “Target position / PA-Move Absolute” area, two target positions can be defined. The “Go to” button allows executing the absolute move to go to the specified target position.

“Motion Configuration Values”

In the “Motion Configuration Values”, the current ends of run and the velocity are displayed in a disabled text box: “Minimum end of run”, “Maximum end of run” and “Velocity”. These ends of run and the velocity can be modified and saved with the “Set” button.

Memorised positions

The combo box allows memorizing the positions get by the “Save Pos.” button. Each of these positions can be renamed or deleted. To execute an absolute move to go to one of these memorized positions, select one item of the combo box and click on “Go to” button. When the mouse moves over to the combo box, the positions of the selected memorized position are shown in an information balloon.

Rename a memorized position: Select an item from the combo box, edit the position name to change it and click on the “Rename” button to save the new position name.


Delete a memorized position: Select an item from the combo box, right-click on the mouse and select the “Delete” menu to delete the selected memorized position.

4.3 Tracking

The Tracking tab accesses the position tracking mode. The tracking position mode uses the mouse.

NOTE

In the tracking mode, the cursor is confined to the tracking position area.

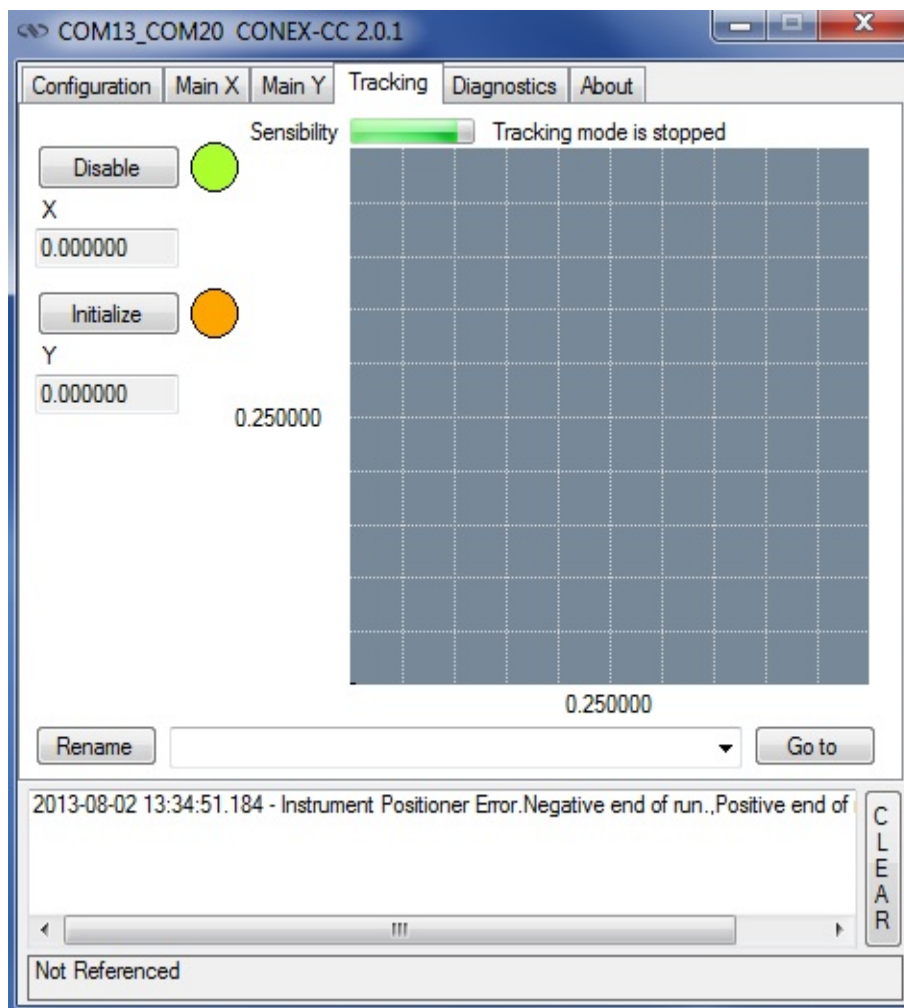

The “Enable/Disable” button executes the next enable command to change the controller status. Its name changes in relation to the controller state. To see the different controller states, refer to the controller state diagram in section 1.3.

An LED icon shows the current controller state. When the mouse hovers over the LED icon, the controller state is displayed inside an information balloon.

Two text boxes display the current positions (X and Y)

The combo box allows memorizing the positions with a mouse double-click. Each of these positions can be renamed or deleted. To execute an absolute move to go to one of these memorized positions, select one item from the combo box and click on “Go to” button. When the mouse moves over to the combo box, the positions of the selected memorized position are showed in an information balloon.


Rename a memorized position: Select an item from the combo box, edit the position name to change it and click on the “Rename” button to save the new position name.

Delete a memorized position: Select an item from the combo box, right-click on the mouse and select the “Delete” menu to delete the selected memorized position.

Tracking panel and mouse

The current position is represented by a black spot.

The amplitudes (X and Y) are defined with the ends of run.


First click (middle mouse button) enters the tracking mode and the mouse cursor position is attached to the current position. As soon as the tracking mode is activated, the cursor is represented by a **hand**  and the CONEX-CC goes to the TRACKING state. Next, each mouse move generates a displacement command. The second click (middle mouse button) exits the tracking mode.

The wheel button increases or decreases the sensitivity..

A right double-click memorizes the current positions (X and Y) in the combo box. Each new memorized position is displayed in the trace.

Default mouse configuration:

- One click:** Enter / Exit the tracking position mode.
- Roll up:** increase zoom factor
- Roll down:** decrease zoom factor

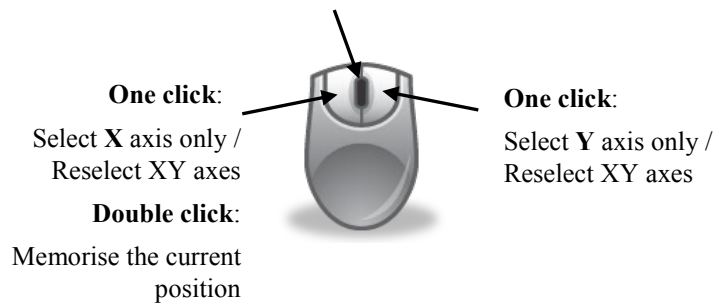


NOTE

The mouse configuration can be modified in the “Configuration” tab.

4.4 Diagnostics


The Diagnostics tab allows the user to enter instrument commands and to view the history of commands that were sent and the responses that were received. This list of commands and the syntax of each command can be found in the user’s manual.

A file of commands can be sent line by line to the controller with the “Send Command file” button.

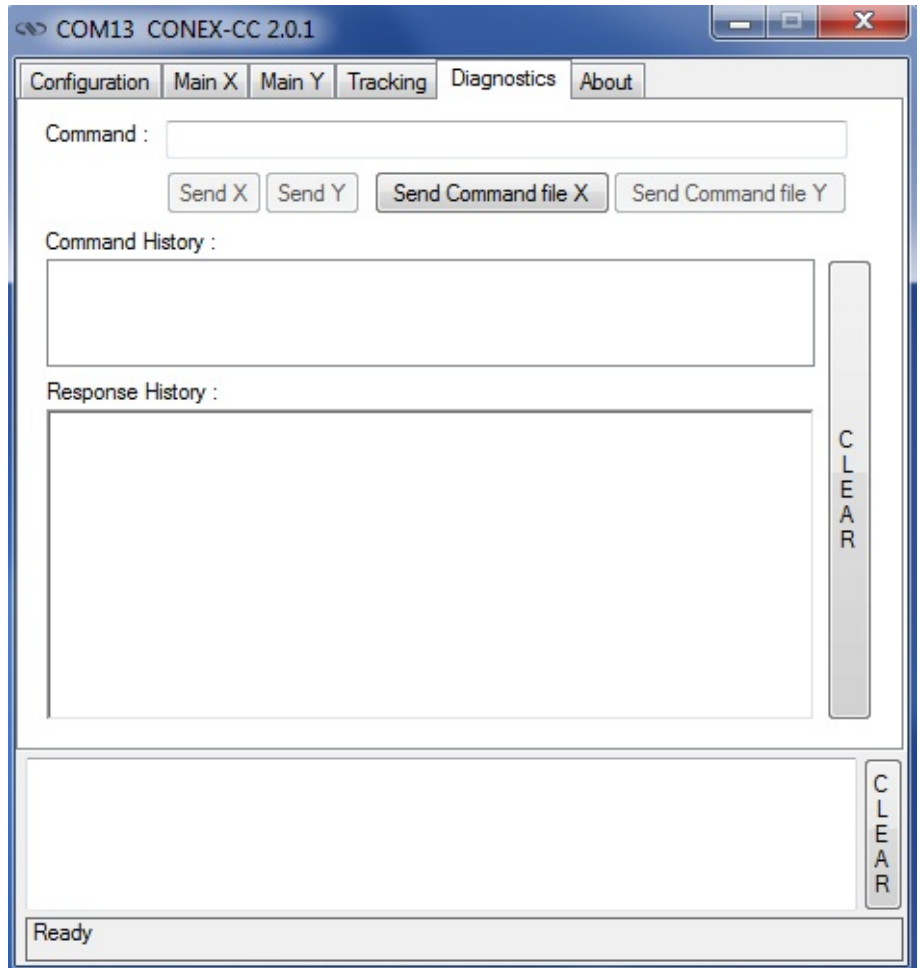

4.5 About

The About tab displays the information about the Controller GUI and the connected instrument. It displays the Controller GUI name, version, and copyright information. It also displays the instrument model, instrument key (serial number) and firmware version for X and Y axes.

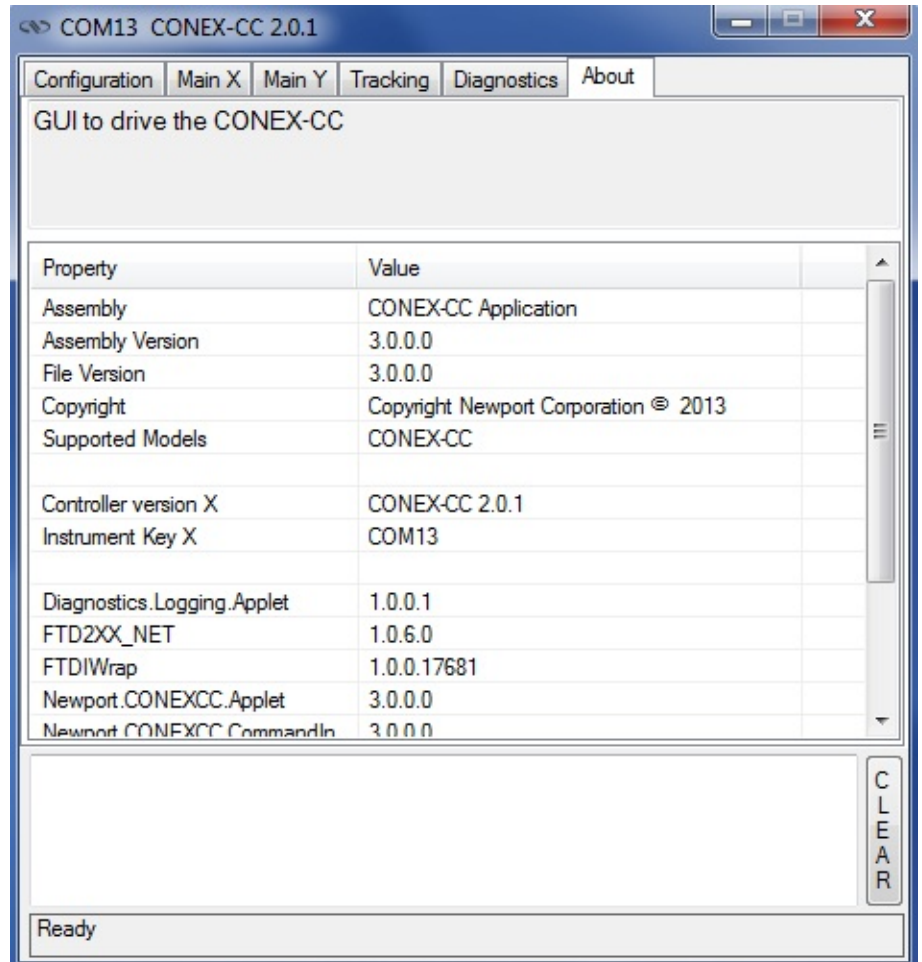



Visit Newport Online at:
www.newport.com

North America & Asia

Newport Corporation
1791 Deere Ave.
Irvine, CA 92606, USA

Sales

Tel.: (800) 222-6440
e-mail: sales@newport.com

Technical Support

Tel.: (800) 222-6440
e-mail: tech@newport.com

Service, RMAs & Returns

Tel.: (800) 222-6440
e-mail: service@newport.com

Europe

MICRO-CONTROLE Spectra-Physics S.A.S
9, rue du Bois Sauvage
91055 Évry CEDEX
France

Sales

Tel.: +33 (0)1.60.91.68.68
e-mail: france@newport.com

Technical Support

e-mail: tech_europe@newport.com

Service & Returns

Tel.: +33 (0)2.38.40.51.55

